


Boditech Quick[™] COVID-19 Ag Nasal

- Rapid detection of SARS-CoV-2 specific antigen
- Simple and quick on-site test
- Nasopharyngeal & Nasal swab available
- All components inclusive



Boditech Quick™ COVID-19 Ag Nasal

• Test procedure

1 1. Nasopharyngeal swab:

insert a sterile swab in the nasal cavity and spin it smoothly in the nasopharynx.



2. Nasal swab:

insert a sterile swab less than 1.5 cm into the nostril and rotate it smoothly. Repeat the collection procedure with the second nostril.




Specimen collection

2 Collect samples with a sterile swab and then put it into the extraction tube. (Spin 5 times)



3 Squeeze and shake to mix 10 times.




4 Assemble a nozzle to the extraction tube.



5 Invert the tube and squeeze it gently to add 4 drops of the sample into the 'sample well' of the test cartridge.



6 Read the result in 10 - 15 minutes.

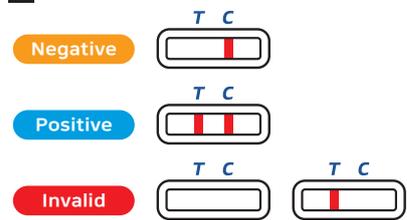

Strong positive results are confirmed in 10 minutes.

• Components

| | |
|------------------------|-------|
| Cartridge | 30 ea |
| Extraction buffer tube | 30 ea |
| Nozzle | 30 ea |

* Note. A nylon swab is excluded from the components of the cartridge box and provided separately.

• Specification

| | |
|------------------------|--|
| Product name | Boditech Quick™ COVID-19 Ag Nasal |
| Cat. No | CFPT-12 |
| Assay type | RDT (Rapid Diagnostic Test) |
| Sample type | Nasopharyngeal swab / Nasal swab |
| Sample prep/extraction | Collecting with nylon swab |
| Target | SARS-CoV-2 Antigen |
| Unit | 30 kits/box |

• Clinical performance

| Nasopharyngeal & Nasal swab | | RT-PCR | | |
|-----------------------------------|----------|----------|----------|-------|
| | | Positive | Negative | Total |
| Boditech Quick™ COVID-19 Ag Nasal | Positive | 76 | 0 | 76 |
| | Negative | 14 | 70 | 84 |
| Total | | 90 | 70 | 160 |
| Positive agreement | | 84.4 % | | |
| Negative agreement | | 100.0 % | | |